



SenTix[®] Sp-T 900(-P)

IDS CUT-IN ELECTRODE WITH POLYMER ELECTROLYTE



a xylem brand

1 General information

Automatic sensor recognition

The sensor electronics with the stored sensor data are in the connecting head of the electrode. The data include, among other things, the sensor type and series number. With each calibration, the calibration data is written in the sensor and the calibration history is recorded (the last 10 calibration procedures). The data is recalled by the meter when the sensor is connected and is used for measurement and for measured value documentation.


Storing the calibration data in the sensor ensures that the correct slope and asymmetry are automatically used if the sensor is operated with different meters. On the other hand, different calibrated sensors can be used with one meter without being recalibrated.

The digital transmission technique guarantees the failure-free communication with the meter even with long connection cables. The sensor firmware can be updated via the meter.

2 Commissioning, measuring, calibration

2.1 Opening and closing the IDS plug connection

This section only applies to variants with IDS plug (SenTix® ... -P).

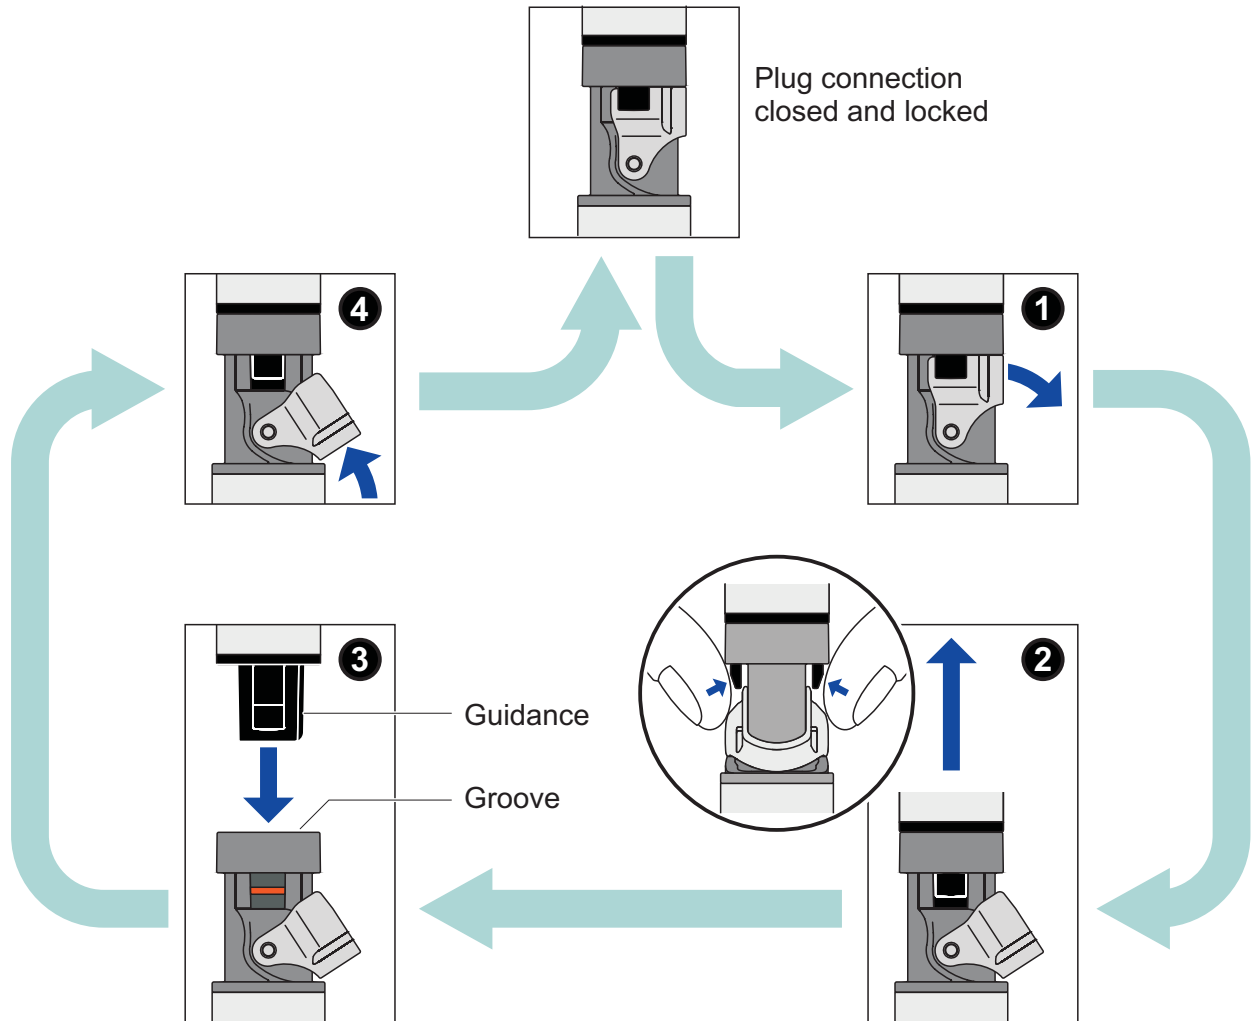

Opening the plug connection

- If necessary, clean the plug connection
- Open the locking device (step 1)
- Use your thumb and index finger to press the clips of the connector together, and pull the connector out of the plug (step 2).

Closing the plug connection

- Make sure that the plug connection is completely dry and clean.
- Align the guidance of the connector with the groove in the plug and insert the connector in the unlocked plug until it catches (step 3).
- Close the locking device (step 4).

2.2 Commissioning

Scope of delivery

- SenTix®Sp-T 900(-P) electrode
- Operating manual

Commissioning

Prepare the electrode for measuring as follows:

- Remove the watering cap from the electrode tip. Possible salt deposits in the area of the watering cap do not affect the measuring characteristics and can easily be removed with deionized water.



Please keep the watering cap. It is required for the electrode to be stored. Always keep the watering cap clean.

- Remove any gas bubbles behind the pH membrane by shaking.
- Connect the electrode to the meter.
- Calibrate the electrode according to the operating manual of the meter and observe the following rules while doing so.


Getting the sensor ready for measuring

SenTix®Sp-T 900	Connect the sensor to the meter. The sensor is immediately ready to measure.
SenTix®Sp-T 900-P	Connect the sensor to a free IDS sensor plug-in position of the multi parameter probe or to an IDS connection of the meter. To open and close the IDS plug-in position please note the section 2.1 OPENING AND CLOSING THE IDS PLUG CONNECTION. The sensor is immediately ready to measure. Connection cables in different lengths to connect the SenTix®Sp-T 900-P sensor to the meter are given in chapter 7 WEAR PARTS AND ACCESSORIES.

2.3 Calibration and measurement: General rules

- Avoid the carryover of any solution (such as sample solution) or measured material from one measurement to the next by taking the following measures:
 - Shortly rinse the containers (such as the calibration containers) with the solution the containers are to be filled with next.
 - Between measurements, rinse the electrode with the solution that follows (e.g. during calibration). Alternatively, you can also rinse the electrode with deionized water and then carefully dab it dry (e.g. for cut-in measurements).
- Make sure that the tip and hole junction are completely covered with the

measured material or solution. The junction is in the area of the bottom end of the shaft (see arrow).



SenTix® Sp-T 900(-P)

Caution: Only the shaft part of the combination electrode may be immersed!

- During cut-in measurements, do not move the electrode and wait for the measured value to become stable.
- For measurements in aqueous solutions, provide approximately the same stirring conditions for measuring as for calibrating.

Subsequent calibrations

The frequency of subsequent calibrations depends on the application. Many meters provide an option where you can enter a calibration interval. After the calibration interval has expired, the meter will automatically remind you of the due calibration.

3 Storage

During short measuring breaks

Immerse the electrode in reference electrolyte (KCl 3 mol/L, Ag⁺ free). Prior to the next measurement, shortly rinse the electrode with the test sample or deionized water.



Prevent contact of the pH membrane to the beaker bottom to avoid scratches on the pH membrane.

Overnight or longer

Put the clean electrode in the watering cap that is filled with reference electrolyte (KCl 3 mol/L, Ag⁺ free).

NOTE

Do not store the pH electrode dry or in deionized water. The electrode could be permanently damaged by this. If the liquid in the watering cap

has dried up, condition the electrode in reference electrolyte (KCl 3 mol/L, Ag+ + free) for at least 24 hours.



During longer storing periods, salt sediments may develop on the watering cap. They do not affect the measuring characteristics and can easily be removed with deionized water when the electrode is put into operation again.

4 Aging

pH electrodes are consumables. Every pH electrode undergoes a natural aging process. With aging, the responding behavior becomes slower and the electrode slope and asymmetry change. Moreover, extreme operating conditions can considerably shorten the lifetime of the electrode. These are:

- Strong acids or lyes, hydrofluoric acid, organic solvents, oils, fats, bromides, sulfides, iodides, proteins
- High temperatures
- High changes in pH and temperature.

The warranty does not cover failure caused by measuring conditions and mechanical damage.

5 Maintenance and cleaning

Cleaning

Remove water-soluble contamination by rinsing with deionized water. Other types of contamination have to be removed as follows while the contact time with the detergents should be kept as short as possible:

Contamination	Cleaning procedure
Fat and oil	Rinse with water containing household washing-up liquid
Lime and hydroxide deposits	Rinse with citric acid (10 % by weight)



Hydrofluoric acid, hot phosphoric acid and strong alkaline solutions destroy the glass membrane.

After cleaning

Rinse the electrode with deionized water and condition it in reference electrolyte solution for at least 1 hour. Then recalibrate the electrode.

6 Technical data

Measurement characteristics	pH measuring range	2.000 ... 13.000
	Allowed temperature range	0 ... 80 °C (32 ... 176 °F)
Accuracy of the IDS measuring technique	Measured parameter	Accuracy (± 1 digit)
	pH	± 0.004
	U [mV]	± 0.2
	T [°C]	± 0.1
General features	Reference electrolyte	Polymer electrolyte, AgCl-free
	Junction	Single hole junction
	Temperature sensor	Integrated NTC 30 (30 kΩ at 25 °C / 77 °F)
Connection cable	Lengths	SenTix®Sp-T 900: 1.5m SenTix®Sp-T 900-P: 1.5 / 6 / 10 / 15 / 25 / 40 / 60 / 100 m
	Diameter	4.3 mm
	Smallest allowed bend radius	Fixed installation: 20 mm Flexible use: 60 mm
	Plug type	Socket, 4 poles
	Shaft dimensions, material	Shaft length
Shaft diameter		15/5 mm
Shaft material		PPE/PS
IDS plug		<ul style="list-style-type: none"> ● Synthetic materials: Glass fiber reinforced Noryl, TPU, TPC-ET, POM, PVC, PEEK, PBT ● O-ring: FPM ● Contacts gold-plated
IDS plug	Connection type	4 pole, watertight plug connection with lock, reverse polarity protected
Storage	With watering cap; filled with KCl 3 mol/L, Ag ⁺ free	

7 Wear parts and accessories

Maintenance equipment

Description	Model	Order no.
Reference electrolyte solution 250 ml to fill the watering cap (KCl 3 mol/l, Ag ⁺ -free)	KCl-250	109 705

Connection cable SenTix®Sp-T 900(-P) - meter

Description	Model	Order no.
IDS connection cable, 1.5 m	AS/IDS-1.5	903 850
IDS connection cable, 3 m	AS/IDS-3	903 851
IDS connection cable, 6 m	AS/IDS-6	903 852
IDS connection cable, 10 m	AS/IDS-10	903 853
IDS connection cable, 15 m	AS/IDS-15	903 854
IDS connection cable, 20 m	AS/IDS-20	903 855
IDS connection cable, 25 m	AS/IDS-25	903 856
IDS connection cable, 40 m	AS/IDS-40	903 857
IDS connection cable, 60 m	AS/IDS-60	903 858
IDS connection cable, 100 m	AS/IDS-100	903 859

8 Disposal

At the end of its operational lifetime, the meter must be returned to the disposal or return system statutory in your country (electronic waste). If you have any questions, please contact your supplier.

We recommend to dispose of the measuring cell as electronic waste.

Xylem |'zīləm|

- 1) The tissue in plants that brings water upward from the roots;
- 2) a leading global water technology company.

We're a global team unified in a common purpose: creating advanced technology solutions to the world's water challenges. Developing new technologies that will improve the way water is used, conserved, and re-used in the future is central to our work. Our products and services move, treat, analyze, monitor and return water to the environment, in public utility, industrial, residential and commercial building services settings. Xylem also provides a leading portfolio of smart metering, network technologies and advanced analytics solutions for water, electric and gas utilities. In more than 150 countries, we have strong, long-standing relationships with customers who know us for our powerful combination of leading product brands and applications expertise with a strong focus on developing comprehensive, sustainable solutions.

For more information on how Xylem can help you, go to www.xylem.com.



Service and Returns:

Xylem Analytics Germany
Sales GmbH & Co. KG
WTW
Am Achalaich 11
82362 Weilheim
Germany

Tel.: +49 881 183-325
Fax: +49 881 183-414
E-Mail wtw.rma@xylem.com
Internet: www.xylemanalytics.com



Xylem Analytics Germany GmbH
Am Achalaich 11
82362 Weilheim
Germany

